

# New Electronic Acupuncture System Using Intelligence

You-Sik Hong, Hongkyun Kim, Cheonshik Kim, Geuk Lee

► **To cite this version:**

You-Sik Hong, Hongkyun Kim, Cheonshik Kim, Geuk Lee. New Electronic Acupuncture System Using Intelligence. James J. Park; Albert Zomaya; Sang-Soo Yeo; Sartaj Sahni. 9th International Conference on Network and Parallel Computing (NPC), Sep 2012, Gwangju, South Korea. Springer, Lecture Notes in Computer Science, LNCS-7513, pp.524-531, 2012, Network and Parallel Computing. <10.1007/978-3-642-35606-3\_62>. <hal-01551368>

**HAL Id: hal-01551368**

**<https://hal.inria.fr/hal-01551368>**

Submitted on 30 Jun 2017

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



# New Electronic Acupuncture System using Intelligence

You-Sik Hong<sup>1</sup>, Hongkyun Kim<sup>2</sup>, Cheonshik Kim<sup>3</sup>, Geuk Lee<sup>4</sup>

<sup>1</sup>School of Information and Communication Engineering, Sang Ji University, Wonju, Kangwon, 220-702, Korea,

<sup>2</sup>Dept. of Electronic Engineering at the Hanbat National University in Taejon, Korea.

<sup>3</sup>Dept. of Computer Science, Sejong University, Seoul, Korea.

<sup>4</sup>Dept. of Information & Communication, Han-nam University, Daejeon, Korea  
yshong@sangji.ac.kr, mipsan@paran.com

**Abstract** In recent years, scientific studies of traditional oriental medicine are accelerating. Furthermore, researches of medical examinations and treatments through collaboration of oriental medicine and western medicine is in progress. This paper will seek for spots on the body suitable for acupuncture using special features that skin impedance values are different. The computer simulation results have shown that Electro-Acupuncture administered by using the medical diagnosis system developed in this study is more effective than the conventional method.

**Keywords:** Pulse wave, Fuzzy Rules, Acupuncture,


## 1 Introduction

In oriental medicine, the term 'pulse' has several meanings. The pulse is considered an important factor in herbal remedies, since observation of a person's pulse rate may reflect their health and illness[1-3]. The observation of heart palpitations is critical as the cessation of a person's heart palpitations classify them as dead. Therefore, the condition of the instant heart change is observed in both western medication and eastern medication, and we can diagnose it by feeling the pulse. Since ancient times, oriental doctors have considered pulse rate as an important data in diagnosis. Accordingly, a doctor who was competent in checking the pulse of their patient was considered a creditable doctor. However, the current blood pressure pulse analyzer may be considered flawed, since it is uncertain whether the blood pressure pulse analyzing sensor is located precisely on the radial artery. Furthermore, the analogue type blood pressure pulse analyzer has the issue of objectifying the blood pressure pulse. Although some people may have the same forearm length, the thickness of their blood vessel may differ, and therefore there is no set of data that is considered reliable enough to judge the accuracy of blood pressure pulse rates. [4-7] In this paper, in order to calculate the best optimal time of Electronic-Acupuncture, it will consider the patient's physical conditions, age conditions and disease conditions[8-12]. As the

computer simulation resulted, Electronic-Acupuncture using the intelligence had proven to be more efficient than the existing method. The composition of this paper is as follows: section 2 discusses the multipad with a built-in Electronic-Acupuncture ; section 3 discusses the fuzzy rules based on pulse wave analysis. Section 4 reports the results of Electronic-Acupuncture simulation and section 5 concludes this paper.

## 2 E-Acupuncture pad with built-in multi-active

What is a multi-pad with a built-active JEUNJACHIM (Electronic-Acupuncture) depending on a patient's current body status? Based on this information, the patient meets the voltage and current self-oscillation. The frequency with the ability to automatically advanced procedure is called JEUNJACHIM. In order to perform these functions simultaneously with the sensing of JEUNJACHIM, one is required to possess the ability to perform surgery, derive accurate analysis from fuzzy logic and process statistical data. Electrical resistance of the body including long-term resistance, internal resistance and the surface can be divided into exposed skin. Resistance of the body when the DC voltage is based on the pure resistive component can be considered only based on the basis, when the impedance of the AC voltage should be considered. That body electrical conductors if you think skin, blood, muscles and other body each part of the voltage and current for the resistive component and capacity components are separated by impedance and its size, the electrical conduction path, the contact voltage, the contact area, and energizing time, is applied differently depending on the frequency may occur.



**Fig. 1.** multipad with a built in electronic acupuncture

Figure 1 illustrates the basic theory of Electronic-Acupuncture. In addition, these changes in a person's age, gender, humidity, temperature, weight and fat accumulation is based on the changes. The requirements when considering the electrical resistance of human skin in general is based on the amount of approximately  $2500\Omega$ . However, the same voltage and current is applied even if the amount of contact area and pain change in resistance over time are different. In the electrical resistance of human body tissues, regardless of the DC and AC power is almost constantly appear if time longer JUAL heat due to temperature rise of tissue resistance is slightly reduced. When the electricity in the human body typically conduct a minimum of power to feel the flow

of the AC voltage is 1mA ~ 2mA for men. In contrast, direct the flow of power is smaller than the stimulus at least five double-road sensing current flow caused by the voltage applied, even though I do not feel the flow of electricity. Thus, in the treatment of **JEUNJACHIM**, electricity is AC rather than DC voltage with the voltage of the aneurysm and the frequency and voltage, over current change as a real hand acupuncture procedures, a small battery that has the same effect as a treatment is likely to be seen. In the experiment, according to AC current that can safely come off as self a man 16mA (60Hz) women 10.5mA (60Hz) is about the human body can withstand DC current is approximately 74mA men for women is approximately 50mA .But it also including a person's body size and weight may appear slightly different depending on the requirements. In this paper, the voltage between 15V ~ 50V AC voltage to the change of 5Hz ~ 1.2Khz and current 500uA ~ 1500uA given in the current experiments were carried out. Figure 2 illustrates the electronic acupuncture circuit

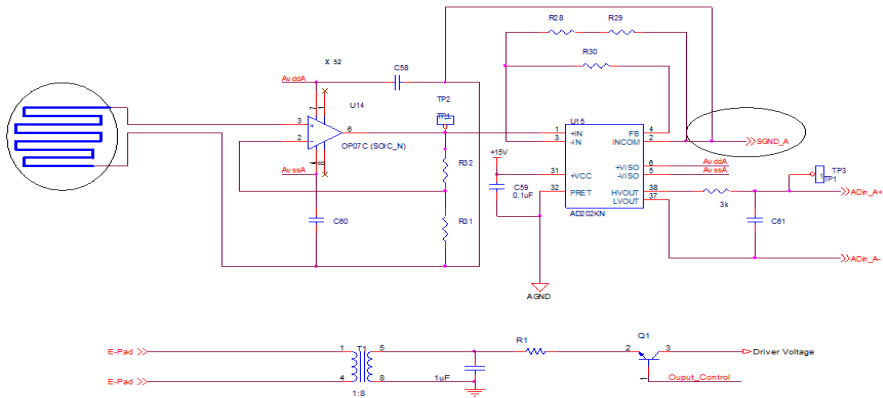


Fig. 2. Electronic acupuncture circuit.

### 3 Fuzzy rules considering the patient's condition

The general algorithm comes to a conclusion of B on the assumption of 'A → B and equals A'. In this case the latter A should be completely consistent with the former A (of conditional clause). This kind of inference is called Modus Ponens and the Fuzzy algorithm is trying to expand as follows which will be called GMP (Generalized Modus Ponens);

Assumption 1: If x equals A, y will be B.

Assumption 2: x equals A'.

Conclusion : y equals B'.

When you use the Fuzzy Rules, the knowledge to judge a patient's health by using the pulse wave will be expressed in Fuzzy R and you will be able to carry out modeling like the following to observe Output (or Symptom) B to clarify Input (or Cause) A.

If you are not careful for actual pulse feeling, often you may be confused that floating

pulse, sliding pulse, and big pulse are powerful while submerging pulse and small pulse aren't. However, some floating pulse, big pulse, and sliding pulse are weak and some submerging pulse and small pulse are strong.

If 4 patients, a, b, c, and d are in their terminal stage, the left figure will be ranging from 0.8 to 1.0 and if in the middle stage, from 0.4 to 0.7 and if in the initial stage, from 0.1 to 0.3. The figure in the middle indicates the patient's physical condition. For example, if a patient is 150 cm high and weighs less than 45 kg, the figure will range from 0.1 to 0.3, if he is 151 - 170 high and weights 46 - 70kg, from 0.4 to 0.7, and if he is 171 - 200 cm high and weights 71 - 130kg, from 0.8 to 1.0. This illustrates the Fuzzy conversion factor to adjust the correlation coefficient in consideration of the weight, age, gender, and physical condition when you analyze patient health condition.

혈압추정계 맥파 측정 DATA SHEET																		
공기압 - 01		진료환자 117.24 순환량 72.888																
측정원자	6.49-31	진료환자 성명	연령성	나이	성별	몸	키	수당치	수당치	수당치	수당치	수당치	수당치	수당치				
순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량	순환량				
1	7.95	118	72	1151	0.250	52.1	0.174	0.130	3.488	-18	0.718	-1.131	0.254	0.969	116	117	72	74
2	7.37	116	72	1095	0.240	54.8	0.182	0.130	3.118	-10	0.781	-1.062	-0.192	0.874	116	110	72	74
3	7.18	116	72	1115	0.250	51.8	0.170	0.130	3.218	-10	0.781	-1.075	-0.211	0.874	116	110	72	74
4	7.82	114	74	1089	0.250	52.1	0.170	0.130	3.371	-10	0.781	-1.089	-0.205	0.864	114	110	74	72
5	7.46	114	74	1078	0.250	53.7	0.186	0.131	3.257	-5	0.807	-0.995	-0.239	0.881	114	110	74	72
6	7.52	114	74	1048	0.247	57.9	0.180	0.134	3.265	-5	0.760	-0.954	-0.244	1.007	114	114	74	68
7	8.00	123	71	1117	0.240	58.2	0.177	0.130	3.425	-6	0.812	-0.889	-0.249	0.814	123	122	71	71
8	8.01	123	71	1174	0.245	51.1	0.167	0.133	3.536	-14	0.777	-0.943	-0.063	0.874	123	131	71	71
9	8.03	123	71	1069	0.244	56.1	0.180	0.130	3.289	-19	0.844	-1.012	0.012	0.871	123	128	71	71
10	8.04	123	71	1095	0.240	58	0.180	0.131	3.291	-11	0.738	-0.951	-0.079	0.864	123	127	71	72
11	8.10	120	67	1089	0.251	53.1	0.185	0.135	3.25	-11	0.768	-1.010	-0.068	0.853	120	119	67	72
12	8.11	120	67	1117	0.255	53.7	0.180	0.137	3.135	-14	0.791	-1.079	-0.118	0.812	120	119	67	74
13	8.13	120	67	1130	0.250	56.3	0.171	0.148	3.475	-17	0.712	-1.129	-0.066	0.818	120	118	67	72
14	8.14	120	67	1201	0.258	49.0	0.171	0.145	3.444	-11	0.764	-1.088	-0.121	0.866	120	114	67	72
15	8.00	118	63	1039	0.240	57.7	0.180	0.130	3.247	-17	0.718	-0.987	-0.204	0.883	118	127	63	72
16	8.02	118	63	0.961	0.240	62.5	0.200	0.119	3.008	-18	0.763	-0.973	-0.087	0.895	118	123	63	72
17	8.02	118	63	0.981	0.247	61.2	0.201	0.132	2.955	-28	0.585	-1.118	-0.160	1.338	118	137	63	69
18	8.03	118	63	1.090	0.240	56	0.180	0.132	3.131	-21	0.696	-1.047	-0.081	0.895	118	121	63	72
19	8.03	117	68	1.111	0.240	54.2	0.180	0.137	3.028	-18	0.719	-1.069	-0.114	0.744	117	118	68	72
20	8.11	122	68	0.950	0.249	63.2	0.210	0.136	2.827	-21	0.640	-1.170	-0.181	1.214	122	124	68	69
21	8.11	122	68	1.027	0.245	59.6	0.195	0.139	3.179	-20	0.712	-1.118	-0.182	1.071	122	120	68	69
22	7.98	117	70	1.012	0.240	59	0.180	0.135	3.229	-6	0.814	-1.047	-0.153	0.844	117	117	70	68
23	7.95	117	70	1.079	0.241	55.6	0.188	0.134	3.130	-7	0.878	-0.955	0.000	0.763	117	117	70	71
24	7.37	113	70	1.050	0.245	57.1	0.197	0.131	3.172	-10	0.812	-0.980	-0.158	0.844	113	118	70	73
25	8.40	127	75	1.107	0.251	54.1	0.182	0.133	3.121	-10	0.755	-1.021	-0.080	0.864	127	128	75	73

Height conditions and age condition




Fig. 3. Patient Health Condition using Fuzzy Rules

The evidences of this kind of hypothesis are atopic disease, acne, and age spot. This skin related troubles happen because the diseased spots have high resistance of electricity. High resistance to electricity means inappropriate oxygen provision therefore the skin disorder occurs in various ways such as atopic disease or age spot. Existing blood pressure pulse analyzing system doesn't consider patient's sex, age, and condition therefore there is an inadequacy of choosing the right amount of pressure to press the needle into patient's skin. It also has a problem of inaccuracy in finding the right acupuncture points. Therefore if a needle is used on an aged patient or a young patient with weak skin it might leave bruises or wounds. In this paper, it tried to solve these problems using intelligent fuzzy rules.

e=R-Y  
Ce=e2-e1

- Where, Y: optimum pulse feeling judgment
- R: Criteria Input
- e: Error
- Ce: Error Displacement
- e2: Current Error

A global priority reflects the importance of an element with respect to the focus of the problem. The derivation of local priorities is carried out through the use of a comparison scale and a pair wise comparison matrix. A comparison matrix for deriving the priority vector

$w^T = (w_1, w_2, w_3, w_4, \dots)$  is associated with 3 elements in a specific level with respect to a single element in a level immediately about it. Such a matrix is denoted by A.

$$A = \begin{bmatrix} w_{1/1} & w_{1/2} & w_{1/3} & w_{1/4} \\ w_{2/1} & w_{2/2} & w_{2/3} & w_{2/4} \\ w_{3/1} & w_{3/2} & w_{3/3} & w_{3/4} \\ w_{4/1} & w_{4/2} & w_{4/3} & w_{4/4} \end{bmatrix}$$

In this matrix every element  $a_{ij}$  is the result of a pair wise comparison denoting the dominance of element  $i$  relative to element  $j$ . A comparison is also being made of the  $j^{\text{th}}$  element with the  $i^{\text{th}}$  element. The fuzzification membership functions in a fuzzy rule base are triangular typed ones defined by equation (1) with  $a, b, u \in U$ . The fuzzy rule base composes of MISO (Multi Input Single Output) typed rule base. Each fuzzy membership function in a fuzzy rule base has a membership value area  $[0,1]$ , and should be normalized in this area.

$$y = \begin{cases} \frac{2}{b-a}(x-a), & a \leq u \leq b, \quad u \in U \\ 0, & \text{otherwise} \end{cases} \quad (1)$$

This interval includes all possible values for the variable in universe of discourse ( $U$ ). All fuzzy sets in a fuzzy rule base have the same support interval  $[a, b]$ . The equation can be represented all types of fuzzy membership functions both fuzzy and non-fuzzy membership functions. The oriental medicine is adopting 4 diagnosis methods such as seeing, hearing, inquiring, and touching but among those is there tongue feeling system in which a doctor will see a patient's tongue for diagnosis. This method has been used to observe the tongue condition or fur deposited on it to diagnose any disease and its kind from the ancient times. Observation of the tongue is mainly used to understand functioning of the heart and spleen. If the tongue fur is white, the corresponding disease is in its initial stage or light, indicating False Symptom, Cold Symptom, and Humid Symptom. If it is yellow, it indicates heat is accumulated in internal organs, most commonly acute fevers.

Fig. 4 illustrates the automatic detection of RGB images which is most similar to the patient's health judgment condition among those tongue feeling images to make the oriental medicine scientific. Moreover, this thesis has developed an algorithm for more accurate judgment of the quantity of tongue furs and the sublingual veins by using the ultraviolet ray and infrared methods.

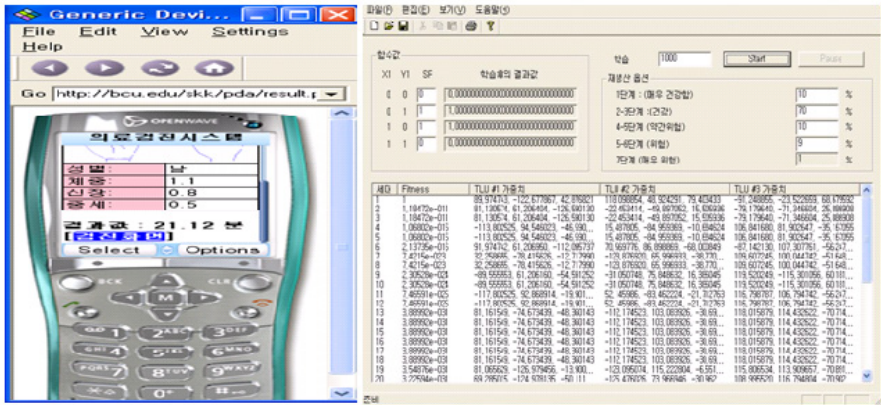


Fig. 4. Pulse wave decision system using fuzzy rules.


Fig. 4 illustrates the Pulse wave decision system using fuzzy rules which depending on the patient's physical condition. In this paper, it is tried to classify the difference in physical characteristics such as thickness of skin and blood vessel, skin impedance, glandular nature of skin in order to come up with an accurate pulse analysis.

#### 4 Simulation

In this paper, in order to solve this kind of problem, it uses compositional inference while using the fuzzy rule. Fuzzy compositional rule of inference is applied to come up with a calibrating constant in order to derive an accurate result (considering the patient's physical condition) in analyzing the blood pressure pulse. In existing method, an oriental doctor infers one pulse wave out of 28 pulse wave and diagnoses the patient. Fuzzy compositional rule of inference is a rule made in order to come up with an inference by using fuzzy production rule which includes fuzzy variables. The form of fuzzy compositional rule of inference is as in the following. Belief of fuzzy composite function: If fuzzy compositional rule of inference is applied in fuzzy production rule then belief of fuzzy evaluation function can't be used. So in order to calculate the belief of fuzzy function, the belief of fuzzy composite function is used.

$$\beta_c = \beta_{comp}(\beta(f), \beta(r)) = \min(\max(\beta(\beta_{fp}), \beta_{rpq}))$$

In here,  $p=1, 2, \dots, m$ ,  $q=1, 2, \dots, n$ .  $m, n$  are the number of each fuzzy thesis in premise and conclusion. Belief of fuzzy union function in type 1 and 2 of fuzzy production rule which are the minimized version of type 5 and 6 can come up with the same node or conclusion using different inference. In this kind of node, same conclusion has two or more different belief of function. In this type of situation, in order to recalculate the belief of fuzzy function, fuzzy union function is used.

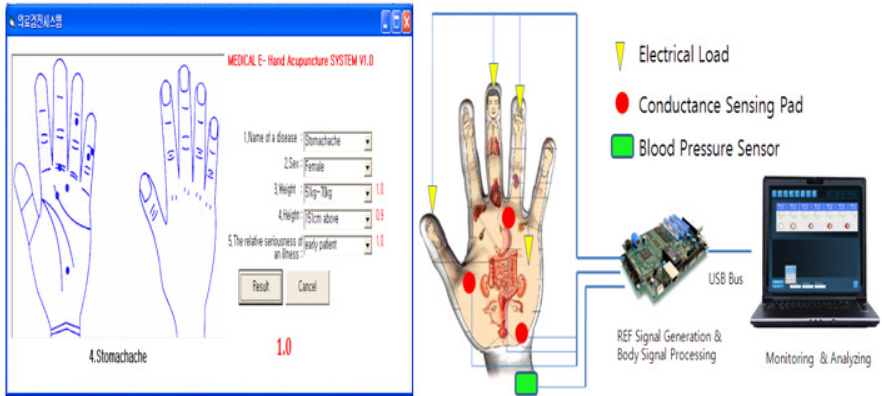

**Fig. 5.** Intelligence DSP Board Firmware

Fig. 5 shows the sequence of DSP Board Firmware. The sequence can be classified into 4 major categories. They are Main Part for main process, Sensor Signal Input & Processor, Data Indexing Processor to create accurate information data on the basis of the sensed data and Fuzzy Logic Driver to create the result data. After power supply, all the register functions of DSP and related memories and variables are initialized. Then, the electric route creation part outputs the electric pattern by the patient condition and A/D and D/A is executed to process the pattern after delivered from the sensor. In this paper, the blood pressure is converted into a form for facilitating judgement via 1st and 2nd derivative and the electrode to measure the conductivity filters each delivered signal to create the input data required by the Fuzzy logic.

## 5 Conclusion

This paper calculates the optimal time for Electronic-Acupuncture using fuzzy rules. In order to calculate the exact acupuncture time, it considers physical condition, illness conditions and age conditions. However, this classification scheme depending on the patient's illness conditions vary greatly. To improve these problems, it adjusts the acupuncture time depending on the patient physical conditions. Since the oriental medicine can check human's health and disease condition by observing the pulse beating condition, the herbal treatment considers the pulse very importantly. The oriental doctor has regarded the pulse as an important data in diagnosis from the past. However, the existing pulse stethoscope was not good enough to confirm if the pulse wave detection sensor was positioned exactly on the aorta radial. Furthermore, it was difficult to feel for accurate pulse of a person with a thick forearm and different body type to the person with a thin forearm. The health judgment by using existing pulse feeling has generated ambiguous problems with accurate judgment due to an oriental doctor's subjective data analysis. In this paper, we applied the Fuzzy algorithm to analyze such a problem and draw an inference from objective data in view of pretreatment and applied the electrical characteristics of pain parts which



respond to acupuncture antidune in view of post-treatment to propose the scientific pulse feeling system algorithm and simulation experiment.

## Acknowledgments

This work was supported by the Security Engineering Research Center, granted by the Korea Ministry of Knowledge Economy.

## References

1. Y. J. Lee, J. Lee, H. J. Lee, H. H. Yoo, E. J. Choi, J. Y. Kim, "Study on the characteristics of blood vessel pulse area using ultrasonic," *Korea Institute of Oriental Medicine researches*, 13(3), pp111 -119, 2007.
2. J. Lee, Y. J. Lee, H. J. Lee, E. J. Choi, J. Y. Kim, "Designing a stabilized process of pulse analyzing method using sigma 6" *Korea Institute of Oriental Medicine researches*, 12(2) pp 85 – 92, 2006.
3. Y. G. Lee, "Diagnostic atlas 2 analyzing pulse" Chungdam books, pp 11 -14, 2003
4. Gunal, S.; Edizkan, R. Subspace based feature selection for pattern recognition. *Information Sciences* 2008.
5. <http://www.etnews.co.kr/etnews/word>.
6. Garg, M. L., Ahson, S. I., and Gupta, D. V., "A Fuzzy Petri-nets for Knowledge Represent- ation and Reasoning," *Information Processing Letters*, 39, pp165-171, 1992.
7. Genrich, H. J., and Lautenbach, K., "System Modelling with High-level Petri Nets," *Theoretical Computer Science*, 13, pp.109-136, 1981.
8. Leung, K. S., and Lam, W., "Fuzzy Concepts in Expert Systems," *IEEE Computer*, Sep., pp.43-56, 1988.
9. Looney, G. C., and Alfize, A. A., "Logical Controls via Boolean Rule Matrix Transformation," *IEEE Trans. on SMC*, Vol. 17, No. 6, Nov./Dec., pp1077-1082, 1987.
10. Looney, G. C., "Fuzzy Petri Nets for Rule- based Decision Making," *IEEE Trans. on SMC*, Vol. 18, No. 1, Jan./Feb., 1988.
11. M. F. O'Rourke, R. P. Kelly, and A. P. Avolio, *The Arterial Pulse*, 1st Ed., Lea & Febiger, Philadelphia, 1992.
12. Gong, Y. Chen, H. Pu, J. Lian, Y.m. Chen, S. "Quantitative investigation on normal pathological tongue shape and correlation analysis between hypertension and syndrome." *China Journal of Traditional Chinese Medicine and Pharmacy* 2005.
13. Gunal, S.; Edizkan, R. "Subspace based feature selection for pattern recognition." *Information Sciences* 2008.
14. You-Sik hong, " Smart Pulse Wave Detection System using Intelligence" *Internatinal conference, ICHIT, LNCS*, 2011